




# Certain<sup>®</sup> Implant System



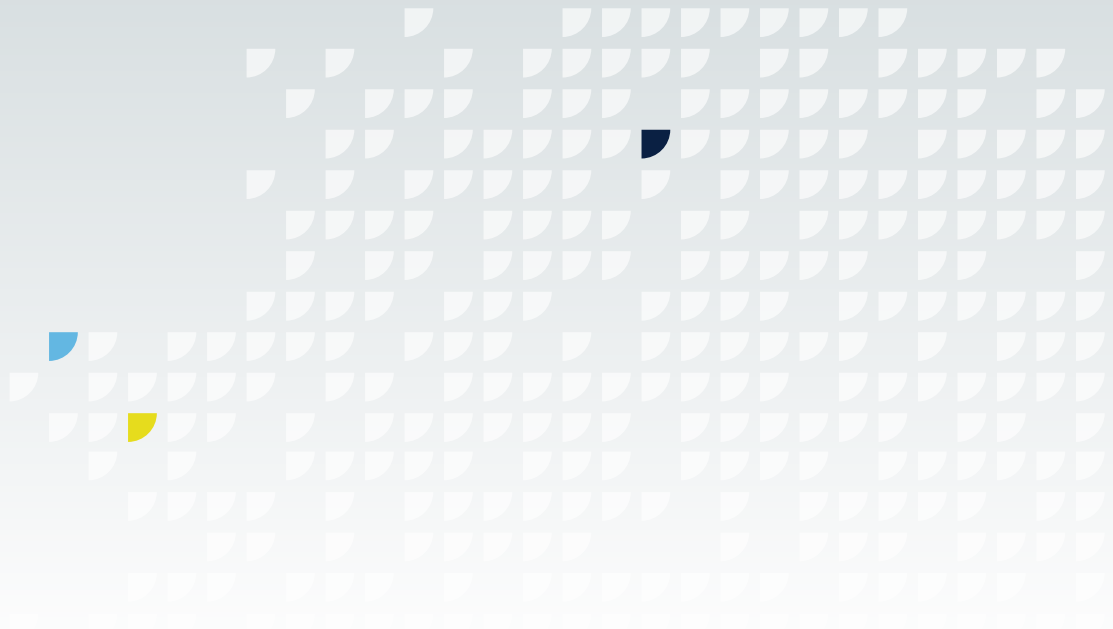

## **IMPORTANT PRODUCT INFORMATION**

### ZimVie Dental Implants

For detailed product information on all ZimVie Dental Implants, refer to the ZimVie Dental Implant IFU ([P-IIS086GI](#)) located at [labeling.zimvie.com](http://labeling.zimvie.com).

### ZimVie Restorative Products

For detailed product information on all ZimVie Restorative Products, refer to the ZimVie Restorative Products IFU ([P-IIS086GR](#)) located at [labeling.zimvie.com](http://labeling.zimvie.com).



# Table of Contents

## Implants

<b>Tapered Certain Internal Connection Implants</b>	<b>4</b>
T3® with DCD® Platform Switched	4
T3 with DCD Non-Platform Switched	4
T3 Platform Switched	4
T3 Non-Platform Switched	4
T3 PRO Platform Switched	4
T3 PRO Non-Platform Switched	4
Full Osseotite® Tapered Certain Prevail®	5
Full Osseotite Tapered Certain	5
Osseotite Tapered Certain	5
<b>Parallel Walled Certain Internal Connection Implants</b>	<b>6</b>
T3 with DCD Platform Switched	6
T3 with DCD Non-Platform Switched	6
T3 Platform Switched	6
T3 Non-Platform Switched	6
Osseotite Parallel Walled Certain	7
Osseotite 2 Parallel Walled Certain	7

## Site Preparation Technologies

<b>Tapered Navigator® System for Guided Surgery</b>	<b>8</b>
Tapered Navigator Surgical Kit	8
Tapered Navigator Tap Kit	10
Tapered Navigator Laboratory Kit	11
<b>Parallel Walled Navigator System for Guided Surgery</b>	<b>12</b>
Parallel Walled Navigator Surgical Kit	12
Parallel Walled Navigator Laboratory Kit	14
<b>Surgical Kits</b>	<b>15</b>
Tapered Implant Surgical Kits	15
Parallel Walled Surgical Kits	18
<b>Surgical Drill System</b>	<b>20</b>
W and H Surgical Drilling Units	20
Advanced Cutting Technology® (ACT®) Twist Drills	21
Quad Shaping Drills For Tapered Implants	21
Miscellaneous Drills	21
<b>Single-Patient Surgical Drills</b>	<b>22</b>
Initiating Drills	22
Quad Shaping Drills	22
ACT Twist Drills	22

<b>Bone Taps</b>	<b>23</b>
Dense Bone Taps for Parallel Walled Implants	23
Dense Bone Taps for Tapered Implants	23
Tapered Implant Depth Indicators	24
Direction Indicators	24
Bone Profilers	25
Tapered Osteotomes	26
Summer Osteotomes	26
Trepphine Burs	26
<b>Miscellaneous Instrumentation</b>	<b>27</b>
Screw Removal Tools	28
<b>Digital Treatment Solutions</b>	<b>29</b>

---


## Restorative Components

<b>Healing Abutments</b>	<b>30</b>
Encode® Emergence	30
EP® One-piece	30
<b>Provisional Restorations</b>	<b>31</b>
PreFormance® Posts	31
Temporary Cylinders	31
<b>Definitive Restorations</b>	<b>32</b>
<b>CAD/CAM Restorations</b>	<b>32</b>
Patient-Specific Abutments	32
GenTek® & GenTek ASC Ti-Bases	32
<b>Castable Restorations</b>	<b>33</b>
UCLA Abutments	33
<b>Cement-Retained Restorations</b>	<b>33</b>
GingiHue® Posts	33
<b>Screw-Retained Restorations</b>	<b>35</b>
Low Profile Abutments	35
<b>Overdenture Restorations</b>	<b>36</b>
OverdenSURE® Abutments	36
<b>Screws</b>	<b>37</b>
Abutment Screws	37
Retaining Screws	37
Waxing Screws and Try-In Screws	37
<b>Drivers, Driver Tips and Miscellaneous Restorative Products</b>	<b>38</b>
<b>Mechanical Driver Kits</b>	<b>39</b>

# Tapered Certain Internal Connection Implants

## T3 WITH DCD PLATFORM SWITCHED IMPLANTS


Commercially Pure Titanium



Length	4/3 mmP	5/4 mmP	6/5 mmP
8.5 mm	BNPT4385	BNPT5485	BNPT6585
10 mm	BNPT4310	BNPT5410	BNPT6510
11.5 mm	BNPT4311	BNPT5411	BNPT6511
13 mm	BNPT4313	BNPT5413	BNPT6513
15 mm	BNPT4315	BNPT5415	BNPT6515

## T3 WITH DCD NON-PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium

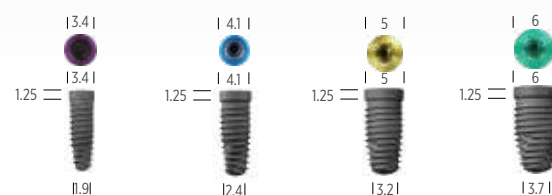

Diameter	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	BNST3285	BNST485	BNST585	BNST685
10 mm	BNST3210	BNST410	BNST510	BNST610
11.5 mm	BNST3211	BNST411	BNST511	BNST611
13 mm	BNST3213	BNST413	BNST513	BNST613
15 mm	BNST3215	BNST415	BNST515	BNST615

## T3 PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium

Length	4/3 mmP	5/4 mmP	6/5 mmP
8.5 mm	BOPT4385	BOPT5485	BOPT6585
10 mm	BOPT4310	BOPT5410	BOPT6510
11.5 mm	BOPT4311	BOPT5411	BOPT6511
13 mm	BOPT4313	BOPT5413	BOPT6513
15 mm	BOPT4315	BOPT5415	BOPT6515


## T3 NON-PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium

Diameter	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	BOST3285	BOST485	BOST585	BOST685
10 mm	BOST3210	BOST410	BOST510	BOST610
11.5 mm	BOST3211	BOST411	BOST511	BOST611
13 mm	BOST3213	BOST413	BOST513	BOST613
15 mm	BOST3215	BOST415	BOST515	BOST615

## T3 PRO PLATFORM SWITCHED IMPLANTS


Commercially Pure Titanium

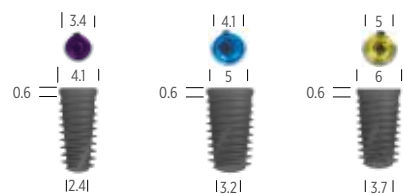

Length	4/3 mmP	5/4 mmP	6/5 mmP
8.5 mm	T3PT4385	T3PT5485	T3PT6585
10 mm	T3PT4310	T3PT5410	T3PT6510
11.5 mm	T3PT4311	T3PT5411	T3PT6511
13 mm	T3PT4313	T3PT5413	T3PT6513
15 mm	T3PT4315	T3PT5415	T3PT6515

## T3 PRO NON-PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium

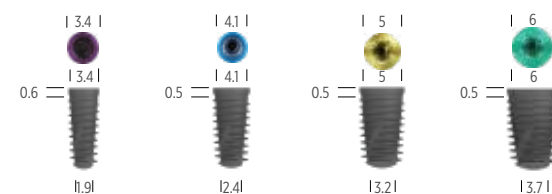


Diameter	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	T3ST3285	T3ST485	T3ST585	T3ST685
10 mm	T3ST3210	T3ST410	T3ST510	T3ST610
11.5 mm	T3ST3211	T3ST411	T3ST511	T3ST611
13 mm	T3ST3213	T3ST413	T3ST513	T3ST613
15 mm	T3ST3215	T3ST415	T3ST515	T3ST615

D = Diameter • P = Restorative Platform




### FULL OSSEOTITE TAPERED CERTAIN PREVAIL

Commercially Pure Titanium

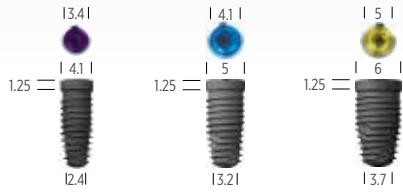

### FULL OSSEOTITE TAPERED CERTAIN

Commercially Pure Titanium

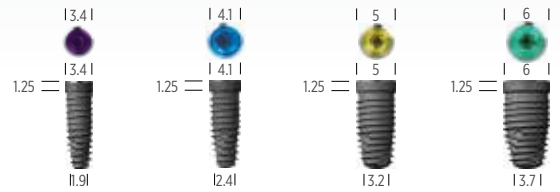

Length	4/3 mmP	5/4 mmP	6/5 mmP
8.5 mm	XIITP4385	XIITP5485	XIITP6585
10 mm	XIITP4310	XIITP5410	XIITP6510
11.5 mm	XIITP4311	XIITP5411	XIITP6511
13 mm	XIITP4313	XIITP5413	XIITP6513
15 mm	XIITP4315	XIITP5415	XIITP6515

3.25 mmD	4 mmD	5 mmD	6.0 mmD
XIFNT3285	XIFNT485	XIFNT585	XIFNT685
XIFNT3210	XIFNT410	XIFNT510	XIFNT610
XIFNT3211	XIFNT411	XIFNT511	XIFNT611
XIFNT3213	XIFNT413	XIFNT513	XIFNT613
XIFNT3215	XIFNT415	XIFNT515	XIFNT615



Cover Screw Flat (included)



\*Non-Flared 4.1 mmP Cover Screw ICS400 is also available.

### OSSEOTITE TAPERED CERTAIN

Commercially Pure Titanium

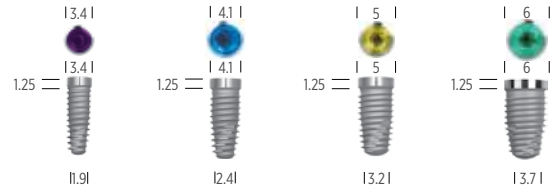

Length	3.25 mmD	4 mmD	5 mmD	6.0 mmD
8.5 mm	INT3285	INT485	INT585	INT685
10 mm	INT3210	INT410	INT510	INT610
11.5 mm	INT3211	INT411	INT511	INT611
13 mm	INT3213	INT413	INT513	INT613
15 mm	INT3215	INT415	INT515	INT615

Cover Screw Flat (included)



\*Non-Flared 4.1 mmP Cover Screw ICS400 is also available.


# Parallel Walled Certain Internal Connection Implants

## T3 WITH DCD PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium




Contemporary Hybrid Surface

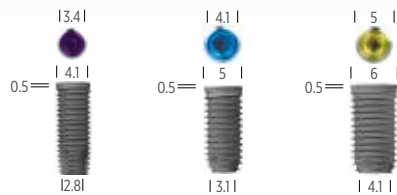

Length	4/3 mmP	5/4 mmP	6/5 mmP
8.5 mm	BNPS4385	BNPS5485	BNPS6585
10 mm	BNPS4310	BNPS5410	BNPS6510
11.5 mm	BNPS4311	BNPS5411	BNPS6511
13 mm	BNPS4313	BNPS5413	BNPS6513
15 mm	BNPS4315	BNPS5415	BNPS6515
18 mm	—	—	—

## T3 WITH DCD NON-PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium

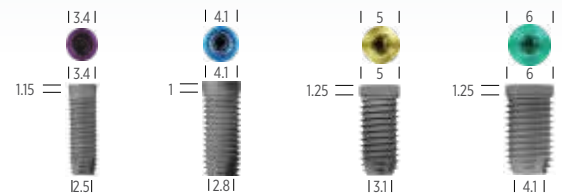

3.25 mmD	4 mmD	5 mmD	6 mmD
BNSS385	BNSS485	BNSS585	BNSS685
BNSS310	BNSS410	BNSS510	BNSS610
BNSS311	BNSS411	BNSS511	BNSS611
BNSS313	BNSS413	BNSS513	BNSS613
BNSS315	BNSS415	BNSS515	BNSS615
BNSS318	BNSS418	—	—

## T3 PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium

Length	4/3 mmP	5/4 mmP	6/5 mmP
8.5 mm	BOPS4385	BOPS5485	BOPS6585
10 mm	BOPS4310	BOPS5410	BOPS6510
11.5 mm	BOPS4311	BOPS5411	BOPS6511
13 mm	BOPS4313	BOPS5413	BOPS6513
15 mm	BOPS4315	BOPS5415	BOPS6515
18 mm	—	—	—



## T3 NON-PLATFORM SWITCHED IMPLANTS

Commercially Pure Titanium

3.25 mmD	4 mmD	5 mmD	6 mmD
BOSS385	BOSS485	BOSS585	BOSS685
BOSS310	BOSS410	BOSS510	BOSS610
BOSS311	BOSS411	BOSS511	BOSS611
BOSS313	BOSS413	BOSS513	BOSS613
BOSS315	BOSS415	BOSS515	BOSS615
BOSS318	BOSS418	—	—

## OSSEOTITE PARALLEL WALLED CERTAIN

Titanium Alloy

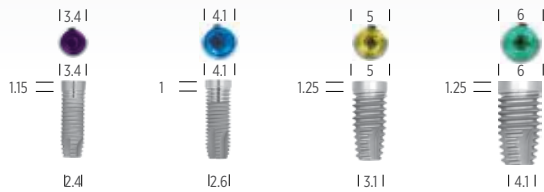


Length	3.25 mmD	4 mmD	5 mmD	6.0 mmD
8.5 mm	IOSS3285	IOSS485	IOSS585	IOSS685
10 mm	IOSS3210	IOSS410	IOSS510	IOSS610
11.5 mm	IOSS3211	IOSS411	IOSS511	IOSS611
13 mm	IOSS3213	IOSS413	IOSS513	IOSS613
15 mm	IOSS3215	IOSS415	IOSS515	IOSS615
18 mm	IOSS3218	IOSS4138	N/A	N/A
20 mm	N/A	IOSS420	N/A	N/A

Cover Screw Flat (included)	3.25 mmD	4 mmD	5 mmD	6.0 mmD
	IMCSF34	ICSF41	ICSF50	ICSF60

\*Non-Flared 4.1 mmP Cover Screw ICS400 is also available.

## OSSEOTITE 2 PARALLEL WALLED CERTAIN

Commercially Pure Titanium

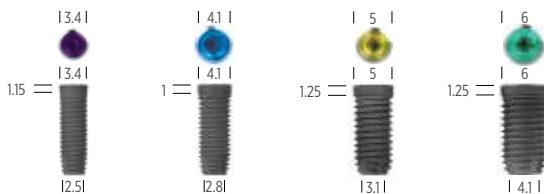

Length	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	XIFOSM385	XIFOSS485	XIFOSS585	XIFOSS685
10 mm	XIFOSM310	XIFOSS410	XIFOSS510	XIFOSS610
11.5 mm	XIFOSM311	XIFOSS411	XIFOSS511	XIFOSS611
13 mm	XIFOSM313	XIFOSS413	XIFOSS513	XIFOSS613
15 mm	XIFOSM315	XIFOSS415	XIFOSS515	XIFOSS615

Cover Screw Flat (included)	3.25 mmD	4 mmD	5 mmD	6 mmD
	IMCSF34	ICSF41	ICSF50	ICSF60

\*Non-Flared 4.1 mmP Cover Screw ICS400 is also available.

# Tapered Navigator System for Guided Surgery

## Site Preparation Technologies

### TAPERED NAVIGATOR SURGICAL KIT

#### For Tapered Implants Including:

- Certain 3.25, 4, and 5 mm Implants
- Prevail 4/3 and 5/4 Implants

The Navigator System helps clinicians transform computer-based planning into practical implant placement with an opportunity for immediate provisionalization.

SGTIKIT

TAPERED NAVIGATOR SURGICAL KIT



#### Features specific to the Navigator System include:

- Depth-specific instrumentation for preparation and implant placement
- Control of hex-orientation to fabricate and deliver provisional restorations immediately following implant placement
- Open architecture compatibility that provides freedom to choose among leading planning software solutions

Description	Item No.	SGTIKIT
Tapered Navigator Surgical Tray	SGTTRAY	•
Tapered Navigator Tissue Punch, 4.1 mmD	SGTTP4	•
Tapered Navigator Tissue Punch, 5 mmD	SGTTP5	•
Tapered Navigator Cortical Perforator, 4.1 mmD - Short	SGTCP4S	•
Tapered Navigator Cortical Perforator, 4.1 mmD - Long	SGTCP4L	•
Tapered Navigator Cortical Perforator, 5 mmD - Short	SGTCP5S	•
Tapered Navigator Cortical Perforator, 5 mmD - Long	SGTCP5L	•
Tapered Navigator Twist Drill, 1.9 mmD x A(L)	SGTD19A	•
Tapered Navigator Twist Drill, 1.9 mmD x B(L)	SGTD19B	•
Tapered Navigator Twist Drill, 1.9 mmD x C(L)	SGTD19C	•
Tapered Navigator Twist Drill, 1.9 mmD x D(L)	SGTD19D	•
Tapered Navigator Twist Drill, 1.9 mmD x E(L)	SGTD19E	•
Tapered Navigator Twist Drill, 1.9 mmD x F(L)	SGTD19F	•
Tapered Navigator Twist Drill, 1.9 mmD x G(L)	SGTD19G	•
Tapered Navigator Countersink Drill, 3.4 mmD - Short	MSGTCD5	•
Tapered Navigator Countersink Drill, 4.1 mmD - Short	SGTCD4S	•
Tapered Navigator Countersink Drill, 5 mmD - Short	SGTCD5S	•
Tapered Navigator Countersink Drill, 3.4 mmD - Long	MSGTCDL	•
Tapered Navigator Countersink Drill, 4.1 mmD - Long	SGTCD4L	•
Tapered Navigator Countersink Drill, 5 mmD - Long	SGTCD5L	•
Tapered Navigator Shaping Drill, 3.25 mmD x 8.5 mmL - Short	MSGTD85S	•
Tapered Navigator Shaping Drill, 3.25 mmD x 10 mmL - Short	MSGTD10S	•
Tapered Navigator Shaping Drill, 3.25 mmD x 11.5 mmL - Short	MSGTD11S	•
Tapered Navigator Shaping Drill, 3.25 mmD x 13 mmL - Short	MSGTD13S	•
Tapered Navigator Shaping Drill, 3.25 mmD x 15 mmL - Short	MSGTD15S	•
Tapered Navigator Shaping Drill, 4.1 mmD x 8.5 mmL - Short	SGTD485S	•
Tapered Navigator Shaping Drill, 4.1 mmD x 10 mmL - Short	SGTD410S	•
Tapered Navigator Shaping Drill, 4.1 mmD x 11.5 mmL - Short	SGTD411S	•
Tapered Navigator Shaping Drill, 4.1 mmD x 13 mmL - Short	SGTD413S	•
Tapered Navigator Shaping Drill, 4.1 mmD x 15 mmL - Short	SGTD415S	•
Tapered Navigator Shaping Drill, 5 mmD x 8.5 mmL - Short	SGTD585S	•





## TAPERED NAVIGATOR SURGICAL KIT (CONTINUED)

Description	Item No.	SGTIKIT
Tapered Navigator Shaping Drill, 5 mmD x 10 mmL - Short	SGTD510S	•
Tapered Navigator Shaping Drill, 5 mmD x 11.5 mmL - Short	SGTD511S	•
Tapered Navigator Shaping Drill, 5 mmD x 13 mmL - Short	SGTD513S	•
Tapered Navigator Shaping Drill, 5 mmD x 15 mmL - Short	SGTD515S	•
Tapered Navigator Shaping Drill, 3.25 mmD x 8.5 mmL - Long	MSGTD85L	•
Tapered Navigator Shaping Drill, 3.25 mmD x 10 mmL - Long	MSGTD10L	•
Tapered Navigator Shaping Drill, 3.25 mmD x 11.5 mmL - Long	MSGTD11L	•
Tapered Navigator Shaping Drill, 3.25 mmD x 13 mmL - Long	MSGTD13L	•
Tapered Navigator Shaping Drill, 3.25 mmD x 15 mmL - Long	MSGTD15L	•
Tapered Navigator Shaping Drill, 4.1 mmD x 8.5 mmL - Long	SGTD485L	•
Tapered Navigator Shaping Drill, 4.1 mmD x 10 mmL - Long	SGTD410L	•
Tapered Navigator Shaping Drill, 4.1 mmD x 11.5 mmL - Long	SGTD411L	•
Tapered Navigator Shaping Drill, 4.1 mmD x 13 mmL - Long	SGTD413L	•
Tapered Navigator Shaping Drill, 4.1 mmD x 15 mmL - Long	SGTD415L	•
Tapered Navigator Shaping Drill, 5 mmD x 8.5 mmL - Long	SGTD585L	•
Tapered Navigator Shaping Drill, 5 mmD x 10 mmL - Long	SGTD510L	•
Tapered Navigator Shaping Drill, 5 mmD x 11.5 mmL - Long	SGTD511L	•
Tapered Navigator Shaping Drill, 5 mmD x 13 mmL - Long	SGTD513L	•
Tapered Navigator Shaping Drill, 5 mmD x 15 mmL - Long	SGTD515L	•
Tapered Navigator Twist Drill Positioning Handle	SGTDPHT	•
Tapered Navigator Reduction Drill Positioning Handle	SGTDPHR	•
Handpiece Connector	MDR10	•
Narrow Right Angle Large Hexed Driver Tip, 24 mmL	RASH3N	•
Posterior Large Hexed Driver, 17 mmL	PHD02N	•
Ratchet Extension, 6 mmL - Short	RE100	•
Ratchet Extension, 15 mmL - Long	RE200	•
Ratchet Wrench	WR150	•
Open End Wrench	CW100	•
Navigator Certain Implant Mount, 3.4 mmD - Short	MSGIIMS	•
Navigator Certain Implant Mount, 3.4 mmD - Long	MSGIIML	•
Navigator Certain Implant Mount, 4.1 mmD - Short	SGIIM4S	•
Navigator Certain Implant Mount, 4.1 mmD - Long	SGIIM4L	•
Navigator Certain Implant Mount, 5 mmD - Short	SGIIM5S	•
Navigator Certain Implant Mount, 5 mmD - Long	SGIIM5L	•
Certain Manual Bone Profiler, 3.4 mmD x 4.1 mmP	IMMBP	•
Certain Manual Bone Profiler, 4.1 mmD x 5 mmP	IMBP4	•
Certain Manual Bone Profiler, 5 mmD x 6 mmP	IMBP5	•

## TAPERED NAVIGATOR TAP KIT

### For Tapered Implants Including:

- Certain 3.25, 4, and 5 mm Implants
- Prevail 4/3 and 5/4 Implants

## TAPERED NAVIGATOR TAP KIT

(Included under SGTIKIT)



Description	Item No.	SGTIKIT
Tapered Navigator Bone Tap Tray	SGTTAPT	•
Tapered Navigator Bone Tap, 3.25 mmD x 8.5 mmL - Short	MSGTT85S	•
Tapered Navigator Bone Tap, 3.25 mmD x 10 mmL - Short	MSGTT10S	•
Tapered Navigator Bone Tap, 3.25 mmD x 11.5 mmL - Short	MSGTT11S	•
Tapered Navigator Bone Tap, 3.25 mmD x 13 mmL - Short	MSGTT13S	•
Tapered Navigator Bone Tap, 3.25 mmD x 15 mmL - Short	MSGTT15S	•
Tapered Navigator Bone Tap, 4.1 mmD x 8.5 mmL - Short	SGTT485S	•
Tapered Navigator Bone Tap, 4.1 mmD x 10 mmL - Short	SGTT410S	•
Tapered Navigator Bone Tap, 4.1 mmD x 11.5 mmL - Short	SGTT411S	•
Tapered Navigator Bone Tap, 4.1 mmD x 13 mmL - Short	SGTT413S	•
Tapered Navigator Bone Tap, 4.1 mmD x 15 mmL - Short	SGTT415S	•
Tapered Navigator Bone Tap, 5 mmD x 8.5 mmL - Short	SGTT585S	•
Tapered Navigator Bone Tap, 5 mmD x 10 mmL - Short	SGTT510S	•
Tapered Navigator Bone Tap, 5 mmD x 11.5 mmL - Short	SGTT511S	•
Tapered Navigator Bone Tap, 5 mmD x 13 mmL - Short	SGTT513S	•
Tapered Navigator Bone Tap, 5 mmD x 15 mmL - Short	SGTT515S	•
Tapered Navigator Bone Tap, 3.25 mmD x 8.5 mmL - Long	MSGTT85L	•
Tapered Navigator Bone Tap, 3.25 mmD x 10 mmL - Long	MSGTT10L	•
Tapered Navigator Bone Tap, 3.25 mmD x 11.5 mmL - Long	MSGTT11L	•
Tapered Navigator Bone Tap, 3.25 mmD x 13 mmL - Long	MSGTT13L	•
Tapered Navigator Bone Tap, 3.25 mmD x 15 mmL - Long	MSGTT15L	•
Tapered Navigator Bone Tap, 4.1 mmD x 8.5 mmL - Long	SGTT485L	•
Tapered Navigator Bone Tap, 4.1 mmD x 10 mmL - Long	SGTT410L	•
Tapered Navigator Bone Tap, 4.1 mmD x 11.5 mmL - Long	SGTT411L	•
Tapered Navigator Bone Tap, 4.1 mmD x 13 mmL - Long	SGTT413L	•
Tapered Navigator Bone Tap, 4.1 mmD x 15 mmL - Long	SGTT415L	•
Tapered Navigator Bone Tap, 5 mmD x 8.5 mmL - Long	SGTT585L	•
Tapered Navigator Bone Tap, 5 mmD x 10 mmL - Long	SGTT510L	•
Tapered Navigator Bone Tap, 5 mmD x 11.5 mmL - Long	SGTT511L	•
Tapered Navigator Bone Tap, 5 mmD x 13 mmL - Long	SGTT513L	•
Tapered Navigator Bone Tap, 5 mmD x 15 mmL - Long	SGTT515L	•

## TAPERED NAVIGATOR LABORATORY KIT

### For Tapered Implants Including:

- Certain 3.25, 4, and 5 mm Implants
- Prevail 4/3 and 5/4 Implants

SGTILKIT

TAPERED NAVIGATOR LABORATORY KIT



Description	Item No.	SGTILKIT
Tapered Navigator Laboratory Tray	SGTLTRAY	•
Navigator Certain Analog Mount, 3.4 mmD - Short	MSGIAMS	•
Navigator Certain Analog Mount, 4.1 mmD - Short	SGIAM4S	•
Navigator Certain Analog Mount, 5 mmD - Short	SGIAM5S	•
Navigator Certain Analog Mount, 3.4 mmD - Long	MSGIAML	•
Navigator Certain Analog Mount, 4.1 mmD - Long	SGIAM4L	•
Navigator Certain Analog Mount, 5 mmD - Long	SGIAM5L	•

# Parallel Walled Navigator System for Guided Surgery

Site Preparation Technologies

## PARALLEL WALLED NAVIGATOR SURGICAL KIT

SGKIT

## PARALLEL WALLED NAVIGATOR SURGICAL KIT

### For Parallel Walled Implants Including:

- Certain 3.25, 4, and 5 mm Implants

The Navigator System helps clinicians transform computer-based planning into practical implant placement with an opportunity for immediate provisionalization.



### Features specific to the Navigator System include:

- Depth-specific instrumentation for preparation and implant placement
- Control of hex-orientation to fabricate and deliver provisional restorations immediately following implant placement
- Open architecture compatibility that provides freedom to choose among leading planning software solutions

Description	Item No.	SGKIT
Navigator Surgical Tray	SGTRAY	•
Navigator Tissue Punch, 4.1 mmD	SGTP4	•
Navigator Tissue Punch, 5 mmD	SGTP5	•
Navigator Starter Drill, 3.4 mmDt	MSGSD	•
Navigator Starter Drill, 3/4 mmD	SGSD34	•
Navigator Starter Drill, 4.1 mmD	SGSD4	•
Navigator Starter Drill, 4/5 mmD	SGSD45	•
Navigator Certain Starter Drill, 5 mmD	SGISD5	•
Navigator Twist Drill, 2 mmD x A(L)	SGD2A	•
Navigator Twist Drill, 2 mmD x B(L)	SGD2B	•
Navigator Twist Drill, 2 mmD x C(L)	SGD2C	•
Navigator Twist Drill, 2 mmD x D(L)	SGD2D	•
Navigator Twist Drill, 2 mmD x E(L)	SGD2E	•
Navigator Twist Drill, 2.75 mmD x A(L)	SGD275A	•
Navigator Twist Drill, 2.75 mmD x B(L)	SGD275B	•
Navigator Twist Drill, 2.75 mmD x C(L)	SGD275C	•
Navigator Twist Drill, 2.75 mmD x D(L)	SGD275D	•
Navigator Twist Drill, 2.75 mmD x E(L)	SGD275E	•
Navigator Twist Drill, 3 mmD x A(L)	SGD3A	•
Navigator Twist Drill, 3 mmD x B(L)	SGD3B	•
Navigator Twist Drill, 3 mmD x C(L)	SGD3C	•
Navigator Twist Drill, 3 mmD x D(L)	SGD3D	•
Navigator Twist Drill, 3 mmD x E(L)	SGD3E	•
Navigator Twist Drill, 3.25 mmD x A(L)	SGD325A	•
Navigator Twist Drill, 3.25 mmD x B(L)	SGD325B	•
Navigator Twist Drill, 3.25 mmD x C(L)	SGD325C	•
Navigator Twist Drill, 3.25 mmD x D(L)	SGD325D	•
Navigator Twist Drill, 3.25 mmD x E(L)	SGD325E	•
Navigator Twist Drill, 3.85 mmD x A(L)	SGD385A	•
Navigator Twist Drill, 3.85 mmD x B(L)	SGD385B	•
Navigator Twist Drill, 3.85 mmD x C(L)	SGD385C	•
Navigator Twist Drill, 4.25 mmD x A(L)	SGD425A	•



## PARALLEL WALLED NAVIGATOR SURGICAL KIT (CONTINUED)

Description	Item No.	SGKIT
Navigator Twist Drill, 4.25 mmD x B(L)	SGD425B	•
Navigator Twist Drill, 4.25 mmD x C(L)	SGD425C	•
Navigator Bone Tap, 3.25 mmD	MSGTAP	•
Navigator Bone Tap, 4.1 mmD	SGTAP4	•
Navigator Bone Tap, 4/5 mmD	SGTAP45	•
Navigator Bone Tap, 5 mmD	SGTAP5	•
Navigator Drill Positioning Handle 1	SGDPH1	•
Navigator Drill Positioning Handle 2	SGDPH2	•
Navigator Drill Positioning Handle 3	SGDPH3	•
Navigator Drill Positioning Handle 4	SGDPH4	•
Navigator Drill Positioning Handle 5	SGDPH5	•
Certain Manual Bone Profiler, 3.4 mmD x 4.1 mmP	IMMBP	•
Certain Manual Bone Profiler, 4.1 mmD x 5 mmP	IMBP4	•
Certain Manual Bone Profiler, 5 mmD x 6 mmP	IMBP5	•
Narrow Right Angle Large Hexed Driver Tip, 24 mmL	RASH3N	•
Open End Wrench	CW100	•
Ratchet Wrench	WR150	•
Handpiece Connector	MDR10	•
Posterior Large Hexed Driver, 17 mmL	PHD02N	•
Ratchet Extension - Short, 6 mmL	RE100	•
Ratchet Extension - Long, 15 mmL	RE200	•
Navigator Certain Implant Mount, 3.4 mmD x 1(L)	MSGIIM1	•
Navigator Certain Implant Mount, 3.4 mmD x 2(L)	MSGIIM2	•
Navigator Certain Implant Mount, 3.4 mmD x 3(L)	MSGIIM3	•
Navigator Certain Implant Mount, 3.4 mmD x 4(L)	MSGIIM4	•
Navigator Certain Implant Mount, 4.1 mmD x 1(L)	SGIIM41	•
Navigator Certain Implant Mount, 4.1 mmD x 2(L)	SGIIM42	•
Navigator Certain Implant Mount, 4.1 mmD x 3(L)	SGIIM43	•
Navigator Certain Implant Mount, 4.1 mmD x 4(L)	SGIIM44	•
Navigator Certain Implant Mount, 5 mmD x 1(L)	SGIIM51	•
Navigator Certain Implant Mount, 5 mmD x 2(L)	SGIIM52	•
Navigator Certain Implant Mount, 5 mmD x 3(L)	SGIIM53	•
Navigator Certain Implant Mount, 5 mmD x 4(L)	SGIIM54	•

The following items are not included in the Navigator Surgical Kit, but can be ordered separately, as needed, through ZimVie Dental Customer Service:

Description	Item No.	Description	Item No.
Navigator Twist Drill, 2 mmD x Y(L)	SGD2Y	Navigator Twist Drill, 3.25 mmD x Y(L)	SGD325Y
Navigator Twist Drill, 2 mmD x Z(L)	SGD2Z	Navigator Twist Drill, 3.25 mmD x Z(L)	SGD325Z
Navigator Twist Drill, 2.75 mmD x Y(L)	SGD275Y	Navigator Twist Drill, 3.85 mmD x Y(L)	SGD385Y
Navigator Twist Drill, 2.75 mmD x Z(L)	SGD275Z	Navigator Twist Drill, 3.85 mmD x Z(L)	SGD385Z
Navigator Twist Drill, 3 mmD x Y(L)	SGD3Y	Navigator Twist Drill, 4.25 mmD x Y(L)	SGD425Y
Navigator Twist Drill, 3 mmD x Z(L)	SGD3Z	Navigator Twist Drill, 4.25 mmD x Z(L)	SGD425Z

D = Diameter • L = Length

## PARALLEL WALLED NAVIGATOR LABORATORY KIT

SGLKIT

PARALLEL WALLED NAVIGATOR LABORATORY KIT



Description	Item No.	SGLKIT
Navigator Laboratory Tray	SGLTRAY	•
Navigator Certain Analog Mount, 3.4 mmD x 1(L)	MSGIAM1	•
Navigator Certain Analog Mount, 3.4 mmD x 2(L)	MSGIAM2	•
Navigator Certain Analog Mount, 3.4 mmD x 3(L)	MSGIAM3	•
Navigator Certain Analog Mount, 3.4 mmD x 4(L)	MSGIAM4	•
Navigator Certain Analog Mount, 4.1 mmD x 1(L)	SGIAM41	•
Navigator Certain Analog Mount, 4.1 mmD x 2(L)	SGIAM42	•
Navigator Certain Analog Mount, 4.1 mmD x 3(L)	SGIAM43	•
Navigator Certain Analog Mount, 4.1 mmD x 4(L)	SGIAM44	•
Navigator Certain Analog Mount, 5 mmD x 1(L)	SGIAM51	•
Navigator Certain Analog Mount, 5 mmD x 2(L)	SGIAM52	•
Navigator Certain Analog Mount, 5 mmD x 3(L)	SGIAM53	•
Navigator Certain Analog Mount, 5 mmD x 4(L)	SGIAM54	•

# Surgical Kits

## Site Preparation Technologies

### TAPERED IMPLANT SURGICAL KITS

**QNTSK40 PREMIUM KIT**



**SLIMKT SLIM KIT - CERTAIN**

**SLIMKTE SLIM KIT - CERTAIN AND EXTERNAL HEX**



Description	Item No.	Premium Kit	Upgrade Kit	Starter (Basic) Kit	Certain/External Hex	Certain
		QNTSK40	QNTSK40U	QNTSK20	SLIMKTE	SLIMKT
Quad Shaping Drill, 3.25 mmD x 8.5 mmL	QSD3285	•	•		•	•
Quad Shaping Drill, 3.25 mmD x 10 mmL	QSD3210	•	•	•	•	•
Quad Shaping Drill, 3.25 mmD x 11.5 mmL	QSD3211	•	•	•	•	•
Quad Shaping Drill, 3.25 mmD x 13 mmL	QSD3213	•	•	•	•	•
Quad Shaping Drill, 3.25 mmD x 15 mmL	QSD3215	•	•			
Quad Shaping Drill, 4 mmD x 8.5 mmL	QSD485	•	•		•	•
Quad Shaping Drill, 4 mmD x 10 mmL	QSD410	•	•	•	•	•
Quad Shaping Drill, 4 mmD x 11.5 mmL	QSD411	•	•	•	•	•
Quad Shaping Drill, 4 mmD x 13 mmL	QSD413	•	•	•	•	•
Quad Shaping Drill, 4 mmD x 15 mmL	QSD415	•	•			
Quad Shaping Drill, 5 mmD x 8.5 mmL	QSD585	•	•			
Quad Shaping Drill, 5 mmD x 10 mmL	QSD510	•	•	•		
Quad Shaping Drill, 5 mmD x 11.5 mmL	QSD511	•	•	•		
Quad Shaping Drill, 5 mmD x 13 mmL	QSD513	•	•	•		
Quad Shaping Drill, 5 mmD x 15 mmL	QSD515	•	•			
Quad Shaping Drill, 6 mmD x 8.5 mmL	QSD685	•	•			
Quad Shaping Drill, 6 mmD x 10 mmL	QSD610	•	•			
Quad Shaping Drill, 6 mmD x 11.5 mmL	QSD611	•	•			
Quad Shaping Drill, 6 mmD x 13 mmL	QSD613	•	•			
Quad Shaping Drill, 6 mmD x 15 mmL	QSD615	•	•			
Dense Bone Tap, 3.25 mmD x 8.5 mmL	NTAP3285	•	•		•	•
Dense Bone Tap, 3.25 mmD x 10 mmL	NTAP3210	•	•	•	•	•
Dense Bone Tap, 3.25 mmD x 11.5 mmL	NTAP3211	•	•	•	•	•
Dense Bone Tap, 3.25 mmD x 13 mmL	NTAP3213	•	•	•	•	•
Dense Bone Tap, 3.25 mmD x 15 mmL	NTAP3215	•	•			
Dense Bone Tap, 4 mmD x 8.5 mmL	NTAP485	•	•		•	•
Dense Bone Tap, 4 mmD x 10 mmL	NTAP410	•	•	•	•	•
Dense Bone Tap, 4 mmD x 11.5 mmL	NTAP411	•	•	•	•	•
Dense Bone Tap, 4 mmD x 13 mmL	NTAP413	•	•	•	•	•
Dense Bone Tap, 4 mmD x 15 mmL	NTAP415	•	•			

## TAPERED IMPLANT SURGICAL KITS (CONTINUED)


Description	Item No.	Premium Kit	Upgrade Kit	Starter (Basic) Kit	Certain/ External Hex	Certain
		QNTSK40	QNTSK40U	QNTSK20	SLIMKTE	SLIMKT
Dense Bone Tap, 5 mmD x 8.5 mmL	NTAP585	•	•			
Dense Bone Tap, 5 mmD x 10 mmL	NTAP510	•	•	•		
Dense Bone Tap, 5 mmD x 11.5 mmL	NTAP511	•	•	•		
Dense Bone Tap, 5 mmD x 13 mmL	NTAP513	•	•	•		
Dense Bone Tap, 5 mmD x 15 mmL	NTAP515	•	•			
Dense Bone Tap, 6 mmD x 8.5 mmL	NTAP685	•	•			
Dense Bone Tap, 6 mmD x 10 mmL	NTAP610	•	•			
Dense Bone Tap, 6 mmD x 11.5 mmL	NTAP611	•	•			
Dense Bone Tap, 6 mmD x 13 mmL	NTAP613	•	•			
Dense Bone Tap, 6 mmD x 15 mmL	NTAP615	•	•			
Tapered Implant Dense Bone Tap Kit Tray	NTAPKT	•	•	•		
Tapered Implant Depth Indicator, 3.25 mmD x 8.5 mmL 3ea.	NTDI3285*	•	•		•	•
Tapered Implant Depth Indicator, 3.25 mmD x 10 mmL	NTDI3210	•	•	•	•	•
Tapered Implant Depth Indicator, 3.25 mmD x 11.5 mmL	NTDI3211	•	•	•	•	•
Tapered Implant Depth Indicator, 3.25 mmD x 13 mmL	NTDI3213	•	•	•	•	•
Tapered Implant Depth Indicator, 3.25 mmD x 15 mmL	NTDI3215	•	•			
Tapered Implant Depth Indicator, 4 mmD x 8.5 mmL 3ea.	NTDI485*	•	•		•	•
Tapered Implant Depth Indicator, 4 mmD x 10 mmL	NTDI410	•	•	•	•	•
Tapered Implant Depth Indicator, 4 mmD x 11.5 mmL	NTDI411	•	•	•	•	•
Tapered Implant Depth Indicator, 4 mmD x 13 mmL	NTDI413	•	•	•	•	•
Tapered Implant Depth Indicator, 4 mmD x 15 mmL	NTDI415	•	•			
Tapered Implant Depth Indicator, 5 mmD x 8.5 mmL 3ea.	NTDI585	•	•			
Tapered Implant Depth Indicator, 5 mmD x 10 mmL	NTDI510	•	•	•		
Tapered Implant Depth Indicator, 5 mmD x 11.5 mmL	NTDI511	•	•	•		
Tapered Implant Depth Indicator, 5 mmD x 13 mmL	NTDI513	•	•	•		
Tapered Implant Depth Indicator, 5 mmD x 15 mmL	NTDI515	•	•			
Tapered Implant Depth Indicator, 6 mmD x 8.5 mmL 3ea.	NTDI685	•	•			
Tapered Implant Depth Indicator, 6 mmD x 10 mmL	NTDI610	•	•			
Tapered Implant Depth Indicator, 6 mmD x 11.5 mmL	NTDI611	•	•			
Tapered Implant Depth Indicator, 6 mmD x 13 mmL	NTDI613	•	•			
Tapered Implant Depth Indicator, 6 mmD x 15 mmL	NTDI615	•	•			
Certain Countersink Drill, 4 mmD	ICD100	•	•	•	•	•
QSD/NTDI Surgical Tray w/Plastic Insert	QNTSKT	•		•		
Open End Wrench	CW100	•		•	•	
Ratchet Wrench	WR150	•		•		
High Torque Indicating Ratchet Wrench	H-TIRW**				•	•
Ratchet Extension (Short), 6 mmL	RE100	•		•	•	•
Ratchet Extension (Long), 15 mmL	RE200	•		•		

\*One (1) each for SLIMKT and SLIMKTE.

\*\*H-TIRW is manufactured by Elos Med Tech and distributed by ZimVie Dental - Packaged Individually.

D = Diameter • L = Length



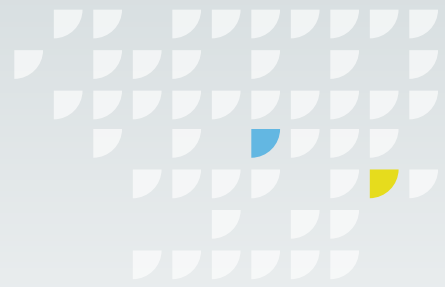

## TAPERED IMPLANT SURGICAL KITS (CONTINUED)

Description	Item No.	Premium Kit	Upgrade Kit	Starter (Basic) Kit	Certain/External Hex	Certain
		QNTSK40	QNTSK40U	QNTSK20	SLIMKTE	SLIMKT
Implant Depth Gauge, 20 mmL	DP020	•				
Narrow Posterior Hexed Driver, 17 mmL	PHD00N	•		•	•	
Posterior Large Hexed Driver, 17 mmL	PHD02N	•		•	•	•
Narrow Right Angle Large Hexed Driver Tip, 24 mmL	RASH3N	•		•		
Direction Indicator, 2 mmD x 10 mmL 3ea.	DI100	•				
Handpiece Connector	MDR10	•			•	•
Implant Mount, 3.4 mmD x 15 mmL	MMC15	•			•	
ACT Pointed Starter Drill	ACTPSD	•			•	•
ACT Reusable Twist Drill, 2 mmD x 10 mmL	ACT2010	•				
ACT Reusable Twist Drill, 2 mmD x 15 mmL	ACT2015	•			•	•
ACT Reusable Twist Drill, 2 mmD x 20 mmL	ACT2020	•		•		
ACT Drill Extension	ACTDE	•			•	•
Internal Connection Universal Placement Driver Tip (Short)	IIPDTUS	•		•	•	•
Internal Connection Universal Placement Driver Tip (Long)	IIPDTUL	•		•		
Certain Universal Ratchet Extension Driver (Short), 6 mmL	IRE100U	•				
Certain Universal Ratchet Extension Driver (Long), 15 mmL	IRE200U	•		•	•	•
Certain Driver Replacement O-Rings, 10-pack	IRORDR	•		•		

## PARALLEL WALLED SURGICAL KITS

PSKT40

PREMIUM KIT



Description	Item No.	Premium Kit	Certain Premium Kit	Starter (Basic) Kit
		PSKT40	PSKT35	PSKT01
Plastic Surgical Tray Organizer	PTT3001	•	•	•
Plastic Tray Organizer for PTT3001	PTT100	•		
ACT Reusable Twist Drill, 2 mmD x 10 mmL	ACT2010	•	•	
ACT Reusable Twist Drill, 2 mmD x 15 mmL	ACT2015	•	•	•
ACT Reusable Twist Drill, 2 mmD x 20 mmL	ACT2020	•	•	
ACT Reusable Twist Drill, 2.75 mmD x 10 mmL	ACT2710	•	•	
ACT Reusable Twist Drill, 2.75 mmD x 15 mmL	ACT2715	•	•	•
ACT Reusable Twist Drill, 2.75 mmD x 20 mmL	ACT2720	•		
ACT Reusable Twist Drill, 3.25 mmD x 10 mmL	ACT3210	•	•	
ACT Reusable Twist Drill, 3 mmD x 15 mmL	ACT3015	•	•	•
ACT Reusable Twist Drill, 3.85 mmD x 20 mmL	ACT3820	•	•	•
ACT Reusable Twist Drill, 4.25 mmD x 8.5 mmL	ACT4285	•	•	
ACT Reusable Twist Drill, 4.25 mmD x 13 mmL	ACT4213	•	•	•
ACT Reusable Twist Drill, 4.25 mmD x 18 mmL	ACT4218	•	•	
ACT Reusable Twist Drill, 4.85 mmD x 8.5 mmL	ACT4885	•	•	
ACT Reusable Twist Drill, 4.85 mmD x 13 mmL	ACT4813	•	•	
ACT Reusable Twist Drill, 4.85 mmD x 18 mmL	ACT4818	•	•	
ACT Reusable Twist Drill, 5.25 mmD x 8.5 mmL	ACT5285	•	•	
ACT Reusable Twist Drill, 5.25 mmD x 13 mmL	ACT5213	•	•	
ACT Reusable Twist Drill, 5.25 mmD x 18 mmL	ACT5218	•	•	
ACT Drill Extension	ACTDE	•	•	•
Countersink/Pilot Drill, 5 mmD	CD500	•	•	•

D = Diameter • L = Length



**PARALLEL WALLED SURGICAL KITS (CONTINUED)**

Description	Item No.	Premium Kit	Certain Premium Kit	Starter (Basic) Kit
		PSKT40	PSKT35	PSKT01
Certain Countersink Drill, 4 mmD	ICD100	•	•	•
Countersink Depth Indicator for ICD100	ICDI100	•	•	•
Countersink Drill, 4.1 mmD	CD100	•		•
Countersink/Pilot Drill, 6 mmD	CD600	•	•	
Pilot Drill, 2 – 3 mmD	PD100	•	•	•
Implant Dense Bone Tap, 3.25 mmD x 18 mmL	MTAP2	•	•	
Implant Dense Bone Tap, 4 mmD x 13 mmL	TAP413	•	•	
Implant Dense Bone Tap, 5 mmD x 13 mmL	TAP53S	•	•	
Implant Dense Bone Tap, 6 mmD x 13 mmL	TAP63S	•		
Osseotite 2 Dense Bone Tap, 5 mmD x 7 – 13 mmL	XTAP53S	•	•	
Osseotite 2 Dense Bone Tap, 6 mmD x 7 – 13 mmL	XTAP63S	•		
Internal Connection Universal Placement Driver Tip (Short)	IIPDTUS	•	•	•
Internal Connection Universal Placement Driver Tip (Long)	IIPDTUL	•	•	•
Certain Universal Ratchet Extension Driver (Short), 6 mmL	IRE100U	•	•	•
Certain Universal Ratchet Extension Driver (Long), 15 mmL	IRE200U	•	•	•
Narrow Small Hexed Hand Driver, 17 mmL	PHD00N	•		•
Narrow Large Hexed Hand Driver, 17 mmL	PHD02N	•	•	•
Narrow Large Hexed Driver, Tip 24 mmL	RASH3N	•	•	•
Driver Tip Replacement O-Rings, 10-pack	IRORDR	•	•	
Handpiece Connector	MDR10	•	•	•
Open End Wrench	CW100	•		•
Ratchet Wrench	WR150	•	•	•
Ratchet Extension (Short), 6 mmL	RE100	•		•
Ratchet Extension (Long), 15 mmL	RE200	•	•	•
Implant Depth Gauge, 20 mmL	DP020	•	•	•
Implant Mount, 3.4 mmD x 15 mmL	MMC15	•		•
Direction Indicator, 2 mmD x 10 mmL 3ea.	DI100	•	•	•
Stainless Steel Round Drill, 2 mmD	RD100	•	•	•

# Surgical Drill System

## Site Preparation Technologies

### W&H SURGICAL DRILLING UNIT AND OSSTELL ISQ MODULE\*

The surgical drill system is appropriate for implantology with its automatic thread cutter function, automatic torque control, and the Osstell ISQ module for measuring implants stability.



Description	Item No.
<b>Drill Systems</b>	
SI-1023 control unit, 230 V	30288000
SI-1015 control unit, 120 V	30289000
<b>Motors</b>	
EM-19 LC electric motor for SI-1015, w/LED & light contacts (LC), 1.8 m cable	30281000
EM-19 electric motor for SI-1015, without LED+ & light contacts (LC), 1.8 m cable	30185000
EM-19 LC electric motor for SI-1015, w/light contacts (LC), 3.5 m cable	30281001
<b>Handpieces</b>	
WS-75 L, contra-angle 20:1, mini LED+ for EM-19 LC motor	30033000
WS-56 L, contra-angle 1:1, mini LED+ for EM-19 LC motor	30040000
WS-56 L G, contra-angle 1:1, self-generating mini LED+	30039000
WS-75 L G, contra-angle 20:1, self-generating mini LED+	30032000
<b>Foot Controls</b>	
S-NW wireless foot control w/CAN dongle; compatible w/SI-1023, SI-1015	30264000
S-NW wireless foot control w/SPI dongle; compatible w/ SI-915 & Piezomed SA-320	30264001
S-N2 foot control w/cable, compatible w/SI-1015, SI-1023	30285000
<b>Accessories</b>	
W&H Ostell ISQ module, for SI-1015 ,SI-1023	30210000
W&H Osstell Measuring Probe	07721100
Wifi dongle CAN-Bus; SI-1015, SI-1023	07759700
Wifi dongle SPI; SI-915 & Piezomed SA-320	07795800
Universal Motor Holder	07721800
W&H Osstell Test Peg	07849900
SmartPeg Mount	07460300
<b>SmartPegs</b>	
W&H SmartPeg Type 1 - 100353, Pack of 5	08009800
W&H SmartPeg Type 4 - 100350, Pack of 5	08010120
W&H SmartPeg Type 15 - 100386, Pack of 5	08009860
W&H SmartPeg Type 26 - 100425, Pack of 5	08009970
W&H SmartPeg Type 27 - 100431, Pack of 5	08009980
W&H SmartPeg Type 30 - 100436, Pack of 5	08010010
W&H SmartPeg Type 32 - 100440, Pack of 5	08010020
W&H SmartPeg Type 33 - 100442, Pack of 5	08010030
W&H SmartPeg Type 34 - 100444, Pack of 5	08010040
W&H SmartPeg Type 35 - 100446, Pack of 5	08010050
W&H SmartPeg Type 45 - 100472, Pack of 5	08010150
W&H SmartPeg Type 60 - 100543, Pack of 5	08010620

\*Not available in all markets.

# Surgical Drill

## Site Preparation Technologies

### ADVANCED CUTTING TECHNOLOGY (ACT) TWIST DRILLS

#### Features include:

- Two-flute design for efficient cutting
- Alternating lines and bands enhance depth mark visibility and drill orientation in the osteotomy
- Matte finish to reduce glare
- Non-Irrigated Reusable



Implant Lengths	Drill Lengths	2 mmD	2.3 mmD	2.75 mmD	3 mmD	3.15 mmD	3.25 mmD	3.85 mmD	4.25 mmD	4.85 mmD	5.25 mmD
7 – 8.5 mm	8.5 mm	–	–	–	–	–	–	–	ACT4285	ACT4885	ACT5285
7 – 10 mm	10 mm	ACT2010	–	ACT2710	ACT3010	ACT3110	ACT3210	ACT3810	–	–	–
7 – 13 mm	13 mm	–	–	–	–	–	–	–	ACT4213	ACT4813	ACT5213
7 – 15 mm	15 mm	ACT2015	–	ACT2715	ACT3015	ACT3115	ACT3215	ACT3815	–	–	–
7 – 18 mm	18 mm	–	–	–	–	–	–	–	ACT4218	ACT4818	ACT5218
7 – 20 mm	20 mm	ACT2020	–	ACT2720	ACT3020	ACT3120	ACT3220	ACT3820	–	–	–

### QUAD SHAPING DRILLS (QSDS) FOR TAPERED IMPLANTS

#### Features include:


- Quad Shaping Drills use stepped depth marks for accuracy in creating the osteotomy
- QSDs have end cutting ability
- QSDs are color-coded for platform recognition

Drill Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	QSD3285	QSD485	QSD585	QSD685
10 mm	QSD3210	QSD410	QSD510	QSD610
11.5 mm	QSD3211	QSD411	QSD511	QSD611
13 mm	QSD3213	QSD413	QSD513	QSD613
15 mm	QSD3215	QSD415	QSD515	QSD615



### MISCELLANEOUS DRILLS

Description	Reusable
Round Drill, 2 mm	RD100
ACT Pointed Starter Drill	ACTPSD
Pilot Drill, 2–3 mm	PD100
Countersink Drill - Certain 4.1 mm	CD100
Countersink/Pilot Drill, 5 mm	CD500
Countersink/Pilot Drill, 6 mm	CD600



# Single-Patient Surgical Drills

## Site Preparation Technologies

### MISCELLANEOUS DRILLS

Description	Disposable
Round Drill, 2 mm	RD100SP
ACT Pointed Starter Drill	ACTPSDSP
Pilot Drill, 2 – 3 mm	PD100SP
Countersink Drill - Certain 4.1 mm	CD100SP
Countersink/Pilot Drill, 5 mm	CD500SP
Countersink/Pilot Drill, 6 mm	CD600SP



### QUAD SHAPING DRILLS

Drill Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	QSD3285SP	QSD485SP	QSD585SP	QSD685SP
10 mm	QSD3210SP	QSD410SP	QSD510SP	QSD610SP
11.5 mm	QSD3211SP	QSD411SP	QSD511SP	QSD611SP
13 mm	QSD3213SP	QSD413SP	QSD513SP	QSD613SP
15 mm	QSD3215SP	QSD415SP	QSD515SP	QSD615SP



### ACT® TWIST DRILLS

Implant Lengths	Drill Lengths	2 mmD	2.3 mmD	2.75 mmD	3 mmD	3.15 mmD	3.25 mmD	3.85 mmD	4.25 mmD	4.85 mmD	5.25 mmD
7 – 8.5 mm	8.5 mm	–	–	–	–	–	–	–	ACT4285SP	ACT4885SP	ACT5285SP
7 – 10 mm	10 mm	ACT2010SP	–	ACT2710SP	ACT3010SP	ACT3110SP	ACT3210SP	ACT3810SP	–	–	–
7 – 13 mm	13 mm	–	–	–	–	–	–	–	ACT4213SP	ACT4813SP	ACT5213SP
7 – 15 mm	15 mm	ACT2015SP	–	ACT2715SP	ACT3015SP	ACT3115SP	ACT3215SP	ACT3815SP	–	–	–
7 – 18 mm	18 mm	–	–	–	–	–	–	–	ACT4218SP	ACT4818SP	ACT5218SP
7 – 20 mm	20 mm	ACT2020SP	–	ACT2720SP	ACT3020SP	ACT3120SP	ACT3220SP	ACT3820SP	–	–	–



# Bone Taps

## Site Preparation Technologies

### DENSE BONE TAPS FOR PARALLEL WALLED IMPLANTS



Implant Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 – 18 mm	MTAP1 (18 mmL)	—	—	—
8.5 – 18 mm	MTAP2 (27 mmL)	—	—	—
7 – 10 mm	—	TAP410	—	—
7 – 13 mm	—	TAP413	—	—
7 – 20 mm	—	TAP420	—	—
6.5/7 – 8.5 mm	—	—	XTAP58S	XTAP68S
6.5/7 – 13 mm	—	—	XTAP53S	XTAP63S
6.5/7 – 18 mm	—	—	XTAP518S	XTAP618S

### DENSE BONE TAPS FOR TAPERED IMPLANTS



Implant Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	NTAP3285	NTAP485	NTAP585	NTAP685
10 mm	NTAP3210	NTAP410	NTAP510	NTAP610
11.5 mm	NTAP3211	NTAP411	NTAP511	NTAP611
13 mm	NTAP3213	NTAP413	NTAP513	NTAP613
15 mm	NTAP3215	NTAP415	NTAP515	NTAP615

### NTAPK DENSE BONE TAP KIT

Note: Kit includes all of the Dense Bone Taps listed above.



## TAPERED IMPLANT DEPTH INDICATORS

### Features include:

- Tapered Implant Depth Indicators (NTDIs) verify the position of the implant platform prior to placement
- NTDIs are color-coded for platform recognition



Implant Lengths	3.25 mmD	4 mmD	5 mmD	6 mmD
8.5 mm	NTDI3285	NTDI485	NTDI585	NTDI685
10 mm	NTDI3210	NTDI410	NTDI510	NTDI610
11.5 mm	NTDI3211	NTDI411	NTDI511	NTDI611
13 mm	NTDI3213	NTDI413	NTDI513	NTDI613
15 mm	NTDI3215	NTDI415	NTDI515	NTDI615

### Also available in a kit:

NTDIK


IMPLANT DEPTH INDICATORS KIT

Note: Kit includes all of the Implant Depth Indicators listed above.



## DIRECTION INDICATORS

Description	Item No.
2 mm/3 mmD x 10 mmL	DI100
2 mm/3 mmD x 15 mmL	DI200
2.3 mm/3 mmD x 10 mmL, Anodized Blue	DI2310
2.3 mm/3 mmD x 15 mmL, Anodized Gold	DI2315
Certain Direction Indicator Kit	IDIKT
Certain Direction Indicator for 4 mmD, 5 mmD, and 6 mmD Implants	ID1001
Certain Direction Indicator for 3.25 mmD Implants	ID1M01

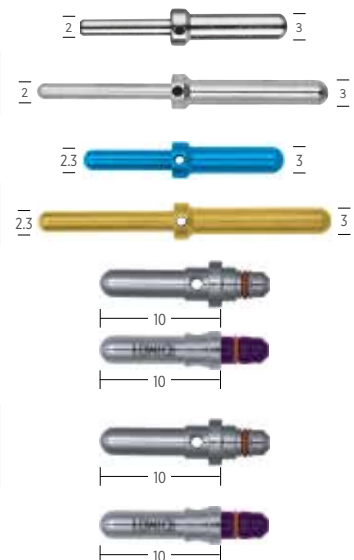

D = Diameter • L = Length



### BONE PROFILERS FOR CERTAIN CONNECTION IMPLANT SYSTEMS\*

Restorative Platform	Emergence Profile	Certain Connection
3.4 mm	3.8 mm	BPC3438
	5.0 mm	BPC3450
4.1 mm	5.0 mm	BPC4150
	6.0 mm	BPC4160
	7.5 mm	BPC4175
5.0 mm	5.5 mm	BPC5055
	6.0 mm	BPC5060
	7.5 mm	BPC5075
6 mm	6.8 mm	BPC6068
	7.5 mm	BPC6075

Note: For Certain Encode Healing Abutments




### BONE PROFILERS FOR CERTAIN LOW PROFILE ABUTMENTS\*

Restorative Platform	Certain Low Profile Abutments
3.4 mm	BPCLP34
4.1 mm	BPCLP41
5.0 mm	BPCLP50



\*Bone Profilers can be used with a contra-angle handpiece or manually. To use manually, please order the Low Torque Indicating Ratchet Wrench Standard ISO 1797 Adapter [item# C9980].

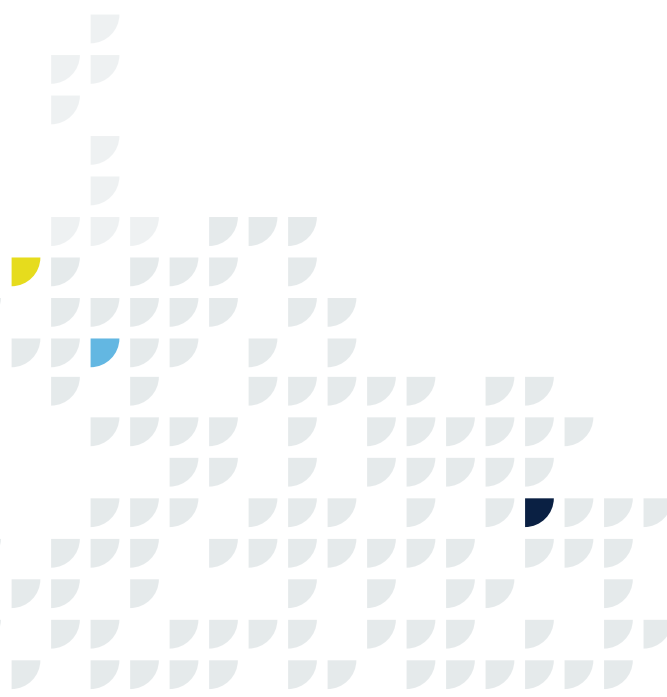

## TAPERED OSTEOTOMES

Available in straight and angled designs for use with Tapered Implants

Description	Item No.
Straight Osseotite Tapered Osteotome Kit	NTOST0
Angled Osseotite Tapered Osteotome Kit	NTOST0A
Straight Osseotite Tapered, 3.25 mmD Osteotome	NTOST3
Straight Osseotite Tapered, 4 mmD Osteotome	NTOST4
Straight Osseotite Tapered, 5 mmD Osteotome	NTOST5
Straight Osseotite Tapered, 6 mmD Osteotome	NTOST6
Angled Osseotite Tapered, 3.25 mmD Osteotome	NTOST3A
Angled Osseotite Tapered, 4 mmD Osteotome	NTOST4A
Angled Osseotite Tapered, 5 mmD Osteotome	NTOST5A
Angled Osseotite Tapered, 6 mmD Osteotome	NTOST6A
Straight Osseotite Tapered Osteotome Tray	NTOSTTRS
Angled Osseotite Tapered Osteotome Tray	NTOSTTRA



## SUMMERS OSTEOTOMES

Available for use with Parallel Walled Implants

Description	Item No.
Summers Osteotome Kit #1-4	OST00
Summers Osteotome Kit #1-5	OST10
Summers Osteotome Kit #1-5, FS	OST20
Summers Osteotome #1	OST01
Summers Osteotome #2	OST02
Summers Osteotome #3	OST03
Summers Osteotome #4	OST04
Summers Osteotome #5	OST05
Summers Osteotome for Future Site	OSTFS
Summers Osteotome System Tray	OSTTR



## TREPINE BURS

Description	Item No.
Trepine Bur, 2 mm Inside Diameter/3 mm Outside Diameter	TRE02
Trepine Bur, 4 mm Inside Diameter/5 mm Outside Diameter	TRE04
Trepine Bur, 5 mm Inside Diameter/6 mm Outside Diameter	TRE05
Trepine Bur, 6 mm Inside Diameter/7 mm Outside Diameter	TRE06
Trepine Bur, 8 mm Inside Diameter/9.3 mm Outside Diameter	TRE08






# Miscellaneous Instrumentation

## Site Preparation Technologies

Description	Item No.
Implant Depth Gauge	DP020
Ratchet Extension, 6 mmL	IRE100U
Ratchet Extension, 15 mmL	IRE200U
Titanium Elevator	TE003

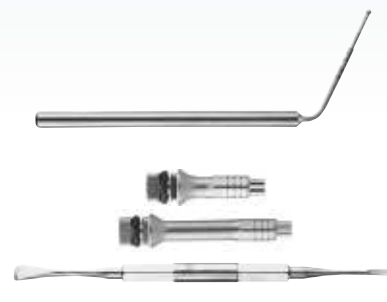

### H-TIRW

### HIGH TORQUE INDICATING RATCHET WRENCH\*


#### Features include:

- The H-TIRW doubles as a conventional ratchet wrench to place implants and as a torque indicator to provide a visual assessment of torque
- Clearly indicates forward and reverse torque of 50-90 Ncm without the need for additional components
- Does not require lubrication or periodic re-calibration. Calibration may be checked by verifying that the arrow is positioned at the first scale mark (0 Ncm)
- Consisting of only two parts, the H-TIRW is easy to prepare for sterilization



\* H-TIRW is manufactured by Elos Medtech AB and distributed by ZimVie Dental.

Description	Item No.
ACT Drill Extension	ACTDE
Certain Implant Placement Driver Tip - Long	IIPDTUL
Certain Implant Placement Driver Tip - Short	IIPDTUS
Gelb Radiographic Depth Gauge Kit - 2 mmD	XDG00
includes:	
2 mmD x 13 mmL	XDG13
2 mmD x 20 mmL	XDG20
Gelb Radiographic Depth Gauge Kit - 2.3 mmD	XDG01
includes:	
2.3 mmD x 13 mmL	XDG2313
2.3 mmD x 20 mmL	XDG2320
Handpiece Connector	MDR10
Tissue Punch, 4.1 mm	TP001
Tissue Punch, 5 mm	TP005
Tissue Punch, 6 mm	TP006

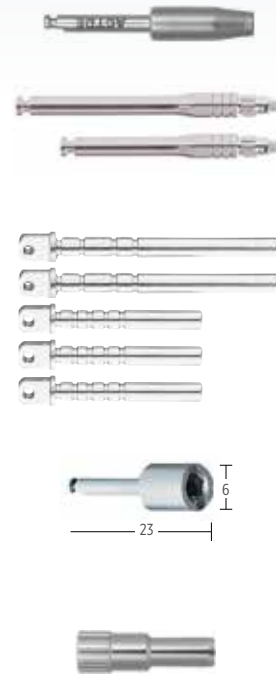


### ISRT10N CERTAIN SCREW REMOVAL TOOLS KIT

**Features include:**

- Extract broken abutment screws from Certain Implants
- Streamlined kit configuration
- Enhanced Extraction Tool durability
- Waxing Screw/Guide Pin verifies the internal threads of the implant
- Up to 15 uses

Certain Drill Guide Handle	ISRT05N
Certain Screw Removal Extraction Tool	ISRT06N
Manual Reversing Drill	USRT07
Certain Waxing Screw / Guide Pin	IWSU30

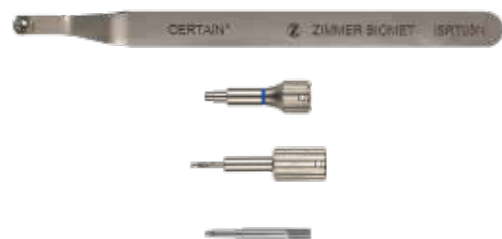

D = Diameter • L = Length



# Digital Treatment Solutions

## Patient-Specific Technologies

### ENCODE IMPRESSION SYSTEM

The Encode Emergence Impression System combines the easy, efficient and proven Encode technology with contemporary emergence profile designs, intuitive codes and pink matte appearance. Eliminate the healing abutment and impression coping or scan body swapping process, while delivering soft tissue healing with natural emergence profile. Patients have a better experience and a beautiful aesthetic outcome as compared to traditional procedures with impression copings.



### EFFICIENT WORKFLOW FOR THE ENTIRE TEAM

The process is simplified with the Encode Emergence Healing Abutment.

### SURGEON

- Efficient, streamlined interoffice processes simplify treatment for the referring dentist.
- Cutting-edge technologies create an improved and more simple treatment process, differentiating the practice to referring dentists and more importantly, to patients.
- The Encode Emergence Impression System makes it easier for your referral base and may increase treatment acceptance.



### LABORATORY

- Potential new customers may lead to increased crown and bridge business.
- There is no need to create a cast, which results in less steps in the treatment process, reducing overhead.
- This unique branding opportunity may grow the volume of your business.



### THE RESULTS: A HIGHLY AESTHETIC DEFINITIVE CAD/CAM ABUTMENT AND VERSATILE GENTEK TI-BASES

### RESTORATIVE CLINICIAN

- Comfort: There is no need to use impression copings, resulting in a less invasive impression procedure for more comfort.
- Fewer Visits: The intraoral scan can be taken by the specialist at the surgical release visit, eliminating a restorative appointment and resulting in less visits to the dentist's office.
- Aesthetic Outcomes: Restorations designed specifically for the patient for better aesthetic outcomes.

GenTek Pre-milled Abutment Blanks



GenTek Ti-Bases

# Healing Abutments

## Restorative Components

### ENCODE EMERGENCE


Restorative Platform	Emergence Profile	Height		
		3 mmH	5 mmH	7 mmH
3.4 mmD	3.8 mmP	IEEHA343	IEEHA345	IEEHA347
	5.0 mmP	IEEHA353	IEEHA355	IEEHA357
4.1 mmD	4.1 mmP	IEEHA443	IEEHA445	IEEHA447
	5.0 mmP	IEEHA453	IEEHA455	IEEHA457
	6.0 mmP	IEEHA463	IEEHA465	IEEHA467
	7.5 mmP	IEEHA473	IEEHA475	IEEHA477
5.0 mmD	5.0 mmP	IEEHA553	IEEHA555	IEEHA557
	6.0 mmP	IEEHA563	IEEHA565	IEEHA567
	7.5 mmP	IEEHA573	IEEHA575	IEEHA577
6.0 mmD	6.0 mmP	IEEHA663	IEEHA665	—
	6.8 mmP	IEEHA6683	IEEHA6685	—
	7.5 mmP	IEEHA673	IEEHA675	—



Dimples on the occlusal provide scanner information for abutment design.

### EP ONE-PIECE

Restorative Platform	Emergence Profile	Collar Height				
		2 mmH	3 mmH	4 mmH	6 mmH	8 mmH
3.4 mmD	3.4 mmP	ISMHA32	ISMHA33	ISMHA34	ISMHA36	—
	3.8 mmP	IMHA32	IMHA33	IMHA34	IMHA36	—
	5 mmP	IMHA352	IMHA353	IMHA354	IMHA356	—
4.1 mmD	4.1 mmP	ISHA42	ISHA43	ISHA44	ISHA46	ISHA48
	5 mmP	ITHA52	ITHA53	ITHA54	ITHA56	ITHA58
5 mmD	6 mmP	—	ITHA63	ITHA64	ITHA66	ITHA68
	5 mmP	ISWHA52	ISWHA53	ISWHA54	ISWHA56	ISWHA58
	5.6 mmP	IWTH52	IWTH53	IWTH54	IWTH56	IWTH58
	6 mmP	IWTH562	IWTH563	IWTH564	IWTH566	IWTH568
6 mmD	6 mmP	ISWHA62	ISWHA63	ISWHA64	ISWHA66	ISWHA68
	6.8 mmP	IWTH62	IWTH63	IWTH64	IWTH66	IWTH68

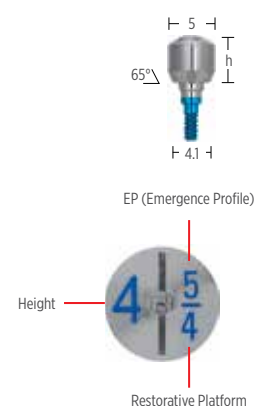

D = Diameter • P = Emergence Profile • H = Collar Height

# Provisional Restorations

## Restorative Components

### COLOR-CODING

Certain Implants and interfacing components are color-coded by restorative platform diameter for easy identification and selection.



### PERFORMANCE POSTS\*

**Material:** PEEK: Titanium Alloy Connection

#### Indications:

- Single- and multiple-unit cement-retained provisional restorations
- Minimum interarch space of 7 mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple-unit restorations will require an evaluation of occlusal forces in lateral and protrusive excursions and masticatory forces to minimize the load on the provisional restorations
- Guided soft-tissue healing of single and multiple-unit restorations of integrated implants



Restorative Platform	Emergence Profile	Collar Height			
		4 mmH		6 mmH	
		Straight	15° Pre-Angled	Straight	15° Pre-Angled
3.4 mmD	3.8 mmP	IMPFP34	IMPAPF34	IMPFP36	IMPAPF36
	5 mmP	IMPFP354	IMPAPF354	IMPFP356	IMPAPF356
4.1 mmD	5 mmP	IPFP454	IPAPF454	IPFP456	IPAPF456
5 mmD	5 mmP	IWFPF554	IPAPF554	IWFPF556	IPAPF556
6 mmD	6 mmP	IWFPF664	IPAPF664	IWFPF666	IPAPF666

### TEMPORARY CYLINDERS\*

#### Indications:

- Single- and multiple-unit screw-retained provisional restorations
- Minimum interarch space of 6 mm
- Maximum angulation of 15°
- Intraoral use limited to 180 days for the PreFormance Temporary Cylinders
- Immediate nonocclusal loading of single-unit provisional restorations
- Multiple-unit restorations will require an evaluation of prosthesis support to minimize the load on the provisional abutments
- Occlusal loading of single- and multiple-unit restorations of integrated implants for guided tissue healing

### PERFORMANCE TEMPORARY CYLINDERS

**Material:** PEEK: Titanium Alloy Connection

Restorative Platform	Description	
	Hexed	Non-Hexed
3.4 mmD	IMPFTC34	IMPFTC32
4.1 mmD	IPFTC41	IPFTC42
5 mmD	IWFTC51	IWFTC52
6 mmD	IWFTC61	IWFTC62



### TITANIUM TEMPORARY CYLINDERS

**Material:** Titanium Alloy Connection

Restorative Platform	Description	
	Hexed	Non-Hexed
3.4 mmD	IMMTC51	—
4.1 mmD	IITCS41	IITCS42
5 mmD	IWTCS51	IWTCS52
6 mmD	IWTCS61	IWTCS62



\*All Provisional Abutments (PreFormance Posts and Temporary Cylinders) include the corresponding Titanium Hexed Screw.

D = Diameter • P = Emergence Profile • H = Collar Height

# Definitive Restorations

## Restorative Components

### CAD/CAM RESTORATIONS

#### GenTek & GenTek ASC Abutments

Material: Titanium

#### Indications:

- Single- and multi-unit CAD/CAM restorations
- Cement- or Screw-retained restorations
- Angled Screw-Channel up to 25° restorations



Seating Surface	Collar Height	GenTek Angulated Screw Channel TiBases	
		Engaging	Non-Engaging
3.4 mm	0.3	ZFX11ZB-CE34ASZ03E	ZFX11ZB-CE34ASZ03N
	1.3	ZFX11ZB-CE34AS13E	ZFX11ZB-CE34AS13N
	2.6	ZFX11ZB-CE34AS26E	-
4.1 mm	0.3	ZFX11ZB-CE41ASZ03E	ZFX11ZB-CE41ASZ03N
	1.3	ZFX11ZB-CE41AS13E	ZFX11ZB-CE41AS13N
	2.6	ZFX11ZB-CE41AS26E	-
5 mm	0.3	ZFX11ZB-CE50ASZ03E	ZFX11ZB-CE50ASZ03N
	1.3	ZFX11ZB-CE50AS13E	ZFX11ZB-CE50AS13N
	2.6	ZFX11ZB-CE50AS26E	-

#### Hexalobular Screwdriver for Hexalobular Retaining Screw\*

Length	Item No.
21 mm	ZFX02HLD21
28 mm	ZFX02HLD28
36 mm	ZFX02HLD36

\*Requires the use of Low Torque Indicating Ratchet Wrench Standard ISO 1797 Adapter [C9980](#)

#### Low Torque Indicating Ratchet Wrench

Description	Item No.
Low Torque Indicating Ratchet Wrench	L-TIRW
L-TIRW Standard ISO 1797 Adapter	C9980



Seating Surface	GenTek TiBases	
	Engaging	Non-Engaging
3.4 mm	ZFX11-ZB-CE-3447-ES	ZFX11-ZB-CE-3447-NES
4.1 mm	ZFX11-ZB-CE-4147-EL	ZFX11-ZB-CE-4147-NEL
5 mm	ZFX11-ZB-CE-5047-EL	ZFX11-ZB-CE-5047-NEL

#### Patient-Specific Abutments

Material: Titanium

#### Indications:

- Single-unit custom abutments
- Cement and screw-retained restorations
- For aesthetic restorations

GenTek Pre-milled Abutment Blanks



Seating Surface	Titanium Pre-milled Abutment Blank <i>incl. Gold-Tite Screw</i>
3.4 mm	ZFX18-ZB-CE-34
4.1, 5.0, 6.0	ZFX18-ZB-CE-4160




## CASTABLE RESTORATIONS

### UCLA Abutments

**Material:** Machined Gold Alloy Cylinder With Plastic Unitube

**Indications:**

- Cement- and screw-retained restorations
- Single- and multi-unit restorations
- Laboratory fabricated custom abutments
- Minimum interarch space of 6 mm
- For aesthetic restorations when tissue is limited
- Maximum angulation correction of 30°



Description	Material	3.4 mmD	4.1 mmD	5 mmD	6 mmD
Hexed	Gold	IMUCG1C*	IGUCA1C*	IWGA51C*	IWGA61C*
Non-Hexed (With Gold-Tite® Large Diameter Screw)	Gold	IMUCG2C	IGUCA2C	IWGA52C	IWGA62C
Non-Hexed (With Ti Large Diameter Screw)	Gold	IMUCG2T	IGUCA2T	IWGA52T	IWGA62T
Non-Hexed (With Gold-Tite Large Diameter Screw)	Castable	IMUCC2C**	IUNAB2C**	IWPC52C**	IWPC62C**
Non-Hexed (With Ti Large Diameter Screw)	Castable	MUCC2T**	IUNAB2T**	IWPC52T**	IWPC62T**

\* UCLA Gold Hexed Abutments do not include the screw. The final Gold-Tite Screw (IUNIHG) or the Titanium Screw (IUNIHT) must be ordered separately.  
 \*\* Not available in the US.

Gold Alloy Cylinder Formulation	
<b>Melting Range</b>	1,400–1,490°C (2550–2710°F)
<b>Solidus</b>	1,400°C
<b>Liquidus</b>	1,490°C
<b>CTE</b>	12.2 x 10 <sup>-6</sup> °K at 500°C

Gold Alloy Cylinder Melting Temperatures		
	Fahrenheit	Celsius
<b>Melting Range</b>	2,552–2,732°F	1,400–1,500°C
<b>Solidus</b>	2,552–2,579°F	1,400–1,415°C
<b>Liquidus</b>	2,714–2,732°F	1,490–1,500°C
<b>CTE</b>	12.2 x 10 <sup>-6</sup> °K at 932°F	12.2 x 10 <sup>-6</sup> °K at 500°C


## CEMENT-RETAINED RESTORATIONS

### GingiHue Posts®

**Material:** Titanium Alloy

**Indications:**

- Single- and multiple-unit porcelain fused-to-metal restorations
- Areas of thin tissue where gingival discoloration is possible
- Preparable to follow gingival contours
- Conventional crown and bridge procedures
- Maximum angulation correction of 15°
- Minimum interarch space of 7 mm



Restorative Platform	Emergence Profile	Collar Height			
		2 mmH		4 mmH	
		Straight	15° Pre-Angled	Straight	15° Pre-Angled
3.4 mmD	3.8 mmP	IMAP32G	IMPAP32G	IMAP34G	IMPAP34G
	5 mmP	IMAP352G	IMPAP352G	IMAP354G	IMPAP354G
4.1 mmD	5 mmP	IAPP452G	IPAP452G	IAPP454G	IPAP454G
	6 mmP	IAPP462G	IPAP462G	IAPP464G	IPAP464G
5 mmD	5 mmP	IWPP552G	IPAP552G	IWPP554G	IPAP554G
	6 mmP	IWPP562G	IPAP562G	IWPP564G	IPAP564G
6 mmD	6 mmP	IWPP662G	IPAP662G	IWPP664G	IPAP664G

\*GingiHue Posts do not include the screw. The final Gold-Tite Screw (IUNISG) must be ordered separately.  
 D = Diameter • P = Emergence Profile • H = Collar Height

## GINGIHUE POST AND UCLA ABUTMENT COMPONENTS

### Pick-Up Impression Coping\*

Restorative Platform	Emergence Profile	Item No.
3.4 mm	3.4 mm	IMIC30
	3.8 mm	IMIC33
	5 mm	IMIC35
4.1 mm	4.1 mm	IIIC41 IIIC42 (non-hexed)
	5 mm	IIIC12
	6 mm	IIIC60
	7.5 mm	IIIC75
	5 mm	IWIP50
5 mm	5.6 mm	IWIP55
	6 mm	IWIP56
	7.5 mm	IWIP57
6 mm	6 mm	IWIP60
	6.8 mm	IWIP66
	7.5 mm	IWIP67



### Twist Lock™ Impression Coping\*\*

Restorative Platform	Emergence Profile	Item No.
3.4 mm	3.8 mm	IMIT33
	5 mm	IMIT35
4.1 mm	4.1 mm	IIIC44
	5 mm	IIIC45
	6 mm	IIIC46
5 mm	7.5 mm	IIIC47
	5 mm	IWIT50
	5.6 mm	IWIT55
6 mm	6 mm	IWIT56
	7.5 mm	IWIT57
	6 mm	IWIT60
	6.8 mm	IWIT66
	7.5 mm	IWIT67



### Laboratory Analog

Restorative Platform	Item No.
3.4 mm	IMMILA
4.1 mm	IILA20
5 mm	IILAW5
6 mm	IILAW6



### Additional Components

Restorative Platform	Item No.
Gold-Tite Screw	IUNIHG
Try-In Screws (5-pack)	IUNITS
Laboratory Abutment Holder	ILTAH57



\* Requires the use of Hex Driver [PHD02N](#), [PHD03N](#) or Driver Tip [RASH3N](#), [RASH8N](#), [IHX12.D](#), [IXL1.2D](#)

\*\*Requires the use of Impression Coping Driver [ICD00](#)


## SCREW-RETAINED RESTORATIONS

### Low Profile Abutments\*

**Material:** Titanium Alloy

**Indications:**

- Single- and multiple-unit screw-retained restorations
- Minimum interarch space of 7.5 mm
- Minimum tissue height of 1 mm
- Angle correction up to 30°

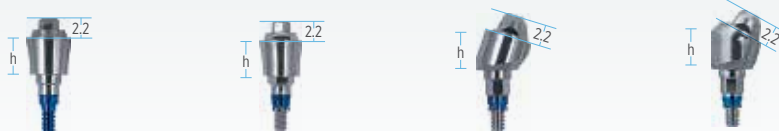

Restorative Platform	Collar Height	Straight (Non-Hexed)	Straight (Hexed)	17° Pre-Angled (Hexed)	30° Pre-Angled (Hexed)
3.4 mmD	1 mm	ILPC341U	ILPC341	—	—
	2 mm	ILPC342U	ILPC342	ILPAC3217	—
	3 mm	ILPC343U	ILPC343	—	ILPAC3330
	4 mm	ILPC344U	ILPC344	ILPAC3417	—
	5 mm	—	—	—	ILPAC3530
4.1 mmD	1 mm	ILPC441U	ILPC441	—	—
	2 mm	ILPC442U	ILPC442	ILPAC4217	—
	3 mm	ILPC443U	ILPC443	—	ILPAC4330
	4 mm	ILPC444U	ILPC444	ILPAC4417	—
	5 mm	—	—	—	ILPAC4530
5 mmD	1 mm	ILPC541U	ILPC541	—	—
	2 mm	ILPC542U	ILPC542	ILPAC5217	—
	3 mm	ILPC543U	ILPC543	—	ILPAC5330
	4 mm	ILPC544U	ILPC544	ILPAC5417	—
	5 mm	—	—	—	ILPAC5530

### Screw-Retained Restorations

Description	4.8 mm Restorative Platform
Pick-Up Impression Coping (hexed)	● LPCPIC1
Pick-Up Impression Coping (non-hexed)	● LPCPIC2
Twist Lock Impression Coping (hexed)	○ LPCTIC1
Twist Lock Impression Coping (non-hexed)	○ LPCTIC2
QuickBridge® Impression Coping	LPCRIC
Laboratory Analog	LPCLA
Temporary Cylinder (hexed)	LPCTC1
Temporary Cylinder (non-hexed)	● LPCTC2
Healing Cap	LPCHC
PreFormance Temp. Cylinder (hexed)	LPCPTC1
PreFormance Temp. Cylinder (non-hexed)	LPCPTC2
QuickBridge	LPCQB
QuickBridge Replacement Cap	LPCQBCAP
Distal Extension	LPCDE

Description	4.8 mm Restorative Platform
Gold Cylinder (hexed)	LPCGC1
Gold Cylinder (non-hexed)	LPCGC2
Castable Cylinder (hexed)	LPCCC1
Castable Cylinder (non-hexed)	LPCCC2
Laser Welded Cylinder	LPCTUCA
Waxing Screw	LPCWS
Retaining Screw	LPCGSH, LPCTSH
Lapping Tool	LPCAMI
Polishing Protector	LPCPP

Abutment Compatibility		
Component	Hexed Abutment	Non-Hexed Abutment
Hexed	Yes	No
Non-Hexed	Yes	Yes

\*Temporary cylinders do not include screw (require LPCGSH or LPCTSH).

● = \* Requires the use of Hex Driver PHD02N, PHD03N or Driver Tip RASH3N, RASH8N, IHX12.D, IXL1.2D

○ = Requires the use of Impression Coping Driver ICDD00

D = Diameter • P = Emergence Profile • H = Collar Height

# Overdenture Restorations

## Restorative Components

### OVERDENSURE ABUTMENTS

#### Material:

Abutment: Titanium Allow with Zirconia Nitride Coating

Housing: Titanium Alloy

Inserts: Nylon















#### Indications:

- Tissue supported removable overdentures on 2-4 implants
- Partially edentulous overdentures with one or more implants
- Limited interarch distance
- Angle correction with up to 40° between divergent implants

Certain® Implant System			
Collar Height	Seating Surface		
	3.4 mm	4.1 mm	5.0 mm
1.0 mm	ODS-CERT301	ODS-CERT401	ODS-CERT501
2.0 mm	ODS-CERT302	ODS-CERT402	ODS-CERT502
3.0 mm	ODS-CERT303	ODS-CERT403	ODS-CERT503
4.0 mm	ODS-CERT304	ODS-CERT404	ODS-CERT504
5.0 mm	ODS-CERT305	ODS-CERT405	ODS-CERT505
6.0 mm	ODS-CERT306	ODS-CERT406	ODS-CERT506



Retention Kit included with each OverdenSURE Abutment



Impression Coping Qty 1	ODS-IC01		Red Retention Insert 40° Qty 4	ODS-RIR4004	
Impression Coping Qty 4	ODS-IC04		Yellow Retention Insert 40° Qty 4	ODS-RIY4004	
Impression Coping Qty 10	ODS-IC010		Green Retention Insert 40° Qty 4	ODS-RIG4004	
Analog Qty 1	ODS-AA01		Retention Housing Cap Qty 1	ODS-RH01	
Analog Qty 4	ODS-AA04		Retention Housing Cap Qty 4	ODS-RH04	
Analog Qty 10	ODS-AA010		Retention Housing Cap Qty 10	ODS-RH010	
Retention Kit 20° Qty 1 Set	ODS-RIKIT001		Blockout Spacer Qty 20	ODS-BS020	
Retention Kit 20° Qty 2 Sets	ODS-RIKIT002		Abutment Driver	ODS-DRVR	
Retention Kit 40° Qty 1 Set	ODS-RIKIT4001		Removal and Insertion Tool	ODS-IRTOOL	
Retention Kit 40° Qty 2 Sets	ODS-RIKIT4002		Abutment Bar Attachment Qty 1	ODS-BARATT01*	
Blue Retention Insert 20° Qty 4	ODS-RIB2004		Abutment Bar Attachment Qty 2	ODS-BARATT02*	
Pink Retention Insert 20° Qty 4	ODS-RIP2004		Abutment Bar Attachment Qty 4	ODS-BARATT04*	
Clear Retention Insert 20° Qty 4	ODS-RIC2004				

\* Does not include Retention Kit



# Screws

## Restorative Components

### ABUTMENT SCREWS

				
	<b>Gold-Tite Screw</b>	<b>Titanium Screw</b>	<b>Large Gold-Tite Screw</b>	<b>Large Titanium Screw</b>
<b>Screws</b>	IUNIHG	IUNIHT	ILRGHG	ILRGHT
<b>Drivers</b>	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N	PHD02N, PHD03N
<b>Driver Tips</b>	IHX1.2D, IXL1.2D	IHX1.2D, IXL1.2D	IHX1.2D, IXL1.2D	IHX1.2D, IXL1.2D
<b>Torque</b>	20 Ncm	20 Ncm	20 Ncm	20 Ncm
<b>For Use With:</b>	Hexed Express, UCLA Abutment, GingiHue Post, GingiHue Post 15°, Hexed Temporary Cylinder	UCLA Abutment, GingiHue Post, GingiHue Post 15°, Hexed Temporary Cylinder	Non -Hexed UCLA Abutment, Non-Hexed Express Abutments, Non-Hexed Temporary Cylinder, Bars	Non -Hexed UCLA Abutment, Non-Hexed Temporary Cylinder, Bars

### RETAINING SCREWS

		
	<b>Low Profile Abutment Gold-Tite Screw</b>	<b>Low Profile Abutment Titanium Screw</b>
<b>Screws</b>	LPCGSH	LPCTSH
<b>Drivers</b>	PHD02N, PHD03N	PHD02N, PHD03N
<b>Driver Tips</b>	IHX1.2D, IXL1.2D	IHX1.2D, IXL1.2D
<b>Torque</b>	10 Ncm	10 Ncm
<b>For Use With:</b>	Low Profile Abutment	Low Profile Abutment

### WAXING SCREWS AND TRY-IN SCREWS

		
	<b>Laboratory Waxing Screw</b>	<b>Hexed Try-In Screw (5-pack)</b>
<b>Screws</b>	IWSU30	IUNITS
<b>Drivers</b>	PHD02N, PHD03N	PHD02N, PHD03N
<b>Driver Tips</b>	IHX1.2D, IXL1.2D	IHX1.2D, IXL1.2D
<b>For Use With:</b>	Pick-Up and Impression Copings, Implant Level Laboratory Procedures	Hexed UCLA Abutment, GingiHue Post, GingiHue Post 15°

# Drivers, Driver Tips, and Miscellaneous Restorative Products

## Restorative Components



Length	Driver	Tip	Driver	Tip	Driver Only
17 mm	PAD00	—	PHD02N	—	ICD00
24 mm	PAD24	RASA3	PHD03N	IHX1.2D	—
30 mm	—	—	—	IXL1.2D	—
<b>For Use With:</b>	Low Profile Abutments		Healing Abutments, Abutment Screws, Certain Cover Screws and Retaining Screws		Twist Lock Transfer Impression Copings

Description	Item No.
Lapping Tool For Castable UCLA Abutment With Guide, 3.4 mmD	IMLT150
Lapping Tool For Castable UCLA Abutment With Guide, 4.1 mmD, 5 mmD	ILT150
Reamer and Handle	IRH600
Certain QuickSeat® Activator Tool	IQSA01
Polishing Protector, UCLA Abutment, 3.4 mmD	IPPMM1
Polishing Protector, UCLA Abutment, 4.1 mmD	IPPIA3
Polishing Protector, UCLA Abutment, 5 mmD	IPPIA5
Polishing Protector, UCLA Abutment, 6 mmD	IPPIA6
Polishing Protector, UCLA Abutment, 3.4 mmD, 4.1 mmD, 5mmD, 6 mmD	ILTAH57
Low Torque Indicating Ratchet Wrench*	L-TIRW
Low Torque Indicating Ratchet Wrench Kit*	L-TIRWK
Standard ISO1797 Adapter	C9980
Short ISO1797 Adapter	C9981
Prosthetic Angle Guide Kit, 15°, 25°, 35°	AG900



\* L-TIRW and L-TIWRK are manufactured by Elos Medtech AB and distributed by ZimVie Dental.

D = Diameter



# Mechanical Driver Kits


## Restorative Components

L-TIRWK LOW TORQUE INDICATING RATCHET WRENCH KIT\*

Description	Item No.
Low Torque Indicating Ratchet Wrench	L-TIRW*
Restorative Torque Tray	RTI2035TR



\*L-TIRW and L-TIWRK are manufactured by Elos Medtech AB and distributed by ZimVie Dental.

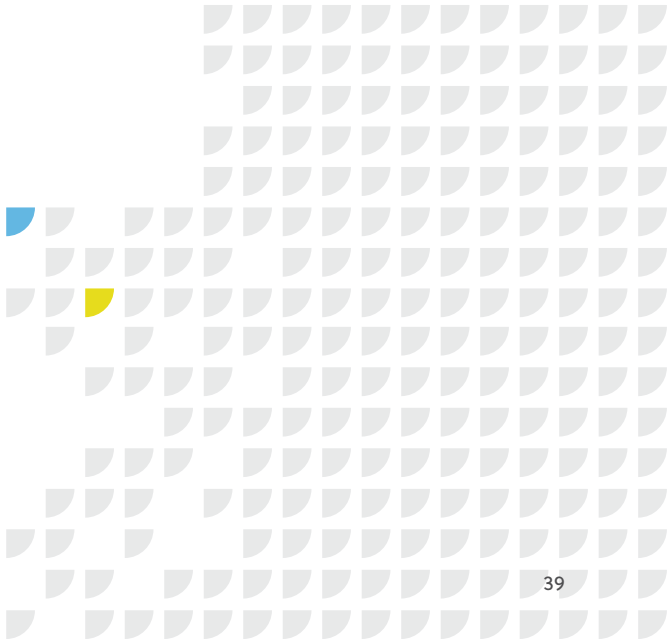

For more information, visit [ZimVie.eu](https://www.zimvie.eu)

**ZimVie Global Headquarters**

4555 Riverside Drive  
Palm Beach Gardens, FL 33410  
Phone: +1-561-776-6700  
Fax: +1-561-776-1272  
[dentalCS@ZimVie.com](mailto:dentalCS@ZimVie.com)

**Biomet 3i (UK & Ireland) Ltd**

Reading Business Centre  
Suite 807, 8th Floor Fountain House  
2 Queens Walk, Reading, Berks  
RG1 7QF, United Kingdom  
Phone (UK): 0800 652 1233  
Phone (Ireland): 1 800 552 752  
[ZV.UKorders@ZimVie.com](mailto:ZV.UKorders@ZimVie.com)



Unless otherwise indicated, as referenced herein, all trademarks and intellectual property rights are the property of ZimVie Inc. or an affiliate; and all products are manufactured by one or more of the dental subsidiaries of ZimVie Inc. (Biomet 3i, LLC, Zimmer Dental, Inc., etc.) and marketed and distributed by ZimVie and its authorized marketing partners. Implantmed is manufactured by W&H Dentalwerk Bürmoos GmbH. Implantmed and W&H are registered trademarks of W&H Dentalwerk Bürmoos GmbH. OverdenSURE is manufactured by Terrats S.L. For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited. This material may not be copied or reprinted without the express written consent of ZimVie. ZVINST0038 REV G 04/24 ©2024 ZimVie. All rights reserved.

